


Class 4 Multi-Parameter EO Indicator

- Conforms to EN ISO 11140-1 Class 4 and is FDA cleared
- Clear and abrupt colour change
- Non-toxic
- Easy to use
- Recordable
- 3 year shelf life
- Lead free

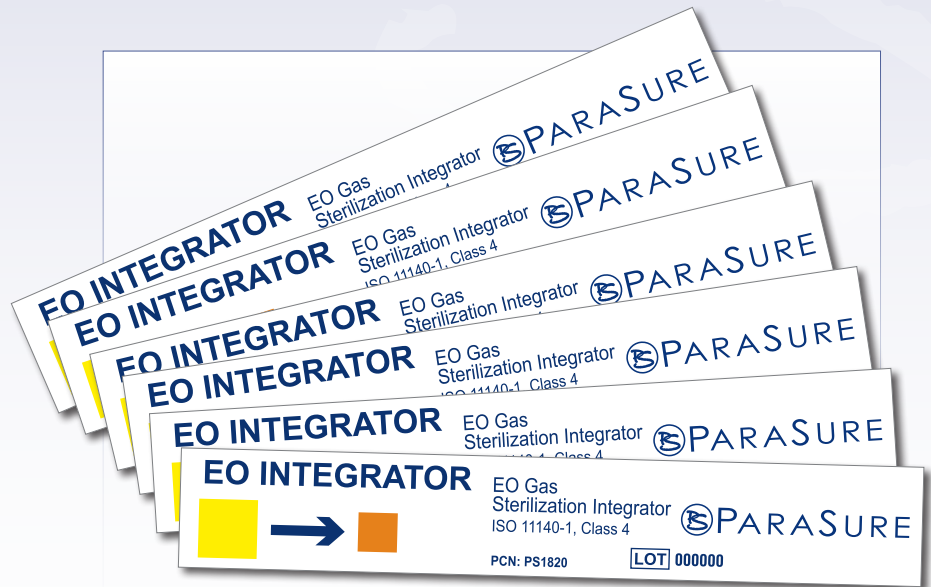

The ParaSure Class 4 Multi-Parameter EO indicator

- The ParaSure EO Integrator has been designed to provide an integrated response to ETO gas Sterilisation. The ETO indicator gives clear visible confirmation that the attainment of all parameters required to attain sterilisation conditions have been met within the sterilisation chamber. When conditions have been met, the indicator changes from yellow to brown.

Order Details

PS1820


Class 4 Multi Parameter
EO indicator

Box of 250


Class 4 Multi-Parameter EO Indicator

TECHNICAL SPECIFICATIONS	
Name:	Class 4 Multi-Parameter EO Indicator
Classification:	EN-ISO 11140-1 Class 4 and FDA cleared
Operating temp:	130°F (54°C)
Time:	45 minutes in EO Resistometer and 60+ minutes in hospital steriliser
Storage conditions:	50 - 100°F (10 - 30°C)
RH:	10% - 60% store as directed in a ziplock moisture barrier bag
Lot no.	yes
Prod date:	yes
Exp date:	3 years
Correct symbols:	in accordance with EN-ISO 11140-1 Class4
Indicator:	yellow to brown
Disp/single use:	yes
Indicator properties:	
Test strip	laminated
Indicator substrate material	80 pound cover
Dimensions	0.625" w x 3.8" L
Extra Information:	
Non-toxic/Lead free	yes
Recordable	yes

EO INTEGRATOR



EO Gas Sterilization Integrator
ISO 11140-1, Class 4



PCN: PS1820 **LOT** 000000

 Before
Original Indicator

Operator: _____

Date: _____

 After
After total process

Address: Squirrels | Kithurst Park |
Storrington | West Sussex | RH20 4JH | England |
Tel: +44 (0) 1903 741390

Warehouse Address: Units B10/B11
Oakendene Estate | Bolney Road | Cowfold |
West Sussex | RH13 8AZ | England